



Certificate of Calibration and Compliance

Manufacturer	:	Viavi Solutions
Model Number	:	Certifier40G
Description	:	NGC-4500-FA
Country of Manufacture	:	MALAYSIA
Serial Number	:	jw20302224
Calibration Report Number	:	20302224-20230703
Calibration Date	:	July 3, 2023
Ambient Temperature	:	(23 ± 3) °C
Relative Humidity	:	30% to 70%

Viavi Solutions certifies that at the time of shipment the above listed instrument as identified by its serial number meets or exceeds all published specifications. It has been calibrated using standards with accuracies that are traceable to the National Institute of Standards and Technology (NIST) or other national laboratories. Accuracies have been derived from accepted values of physical constants, or have been derived by ratio type of self-calibration technique.

Calibration Interval:

The instrument has a calibration cycle of 12 months. Calibration does not deteriorate during storage prior to putting the instrument in active use. Calibration cycle of the instrument can be considered to start on the date the instrument was purchased by end user. First re-calibration will become due 12 months from that date.

Certificate Date

July 3, 2023

Viavi Solutions
Viavisolutions.com



Certificate of Calibration and Compliance

Manufacturer	:	Viavi Solutions
Model Number	:	Certifier40G
Description	:	NGC-4500-FA
Country of Manufacture	:	MALAYSIA
Serial Number	:	jw20302223
Calibration Report Number	:	20302223-20230703
Calibration Date	:	July 3, 2023
Ambient Temperature	:	(23 ± 3) °C
Relative Humidity	:	30% to 70%

Viavi Solutions certifies that at the time of shipment the above listed instrument as identified by its serial number meets or exceeds all published specifications. It has been calibrated using standards with accuracies that are traceable to the National Institute of Standards and Technology (NIST) or other national laboratories. Accuracies have been derived from accepted values of physical constants, or have been derived by ratio type of self-calibration technique.

Calibration Interval:

The instrument has a calibration cycle of 12 months. Calibration does not deteriorate during storage prior to putting the instrument in active use. Calibration cycle of the instrument can be considered to start on the date the instrument was purchased by end user. First re-calibration will become due 12 months from that date.

Certificate Date

July 3, 2023



Viavi Solutions
Viavisolutions.com



Serial No. jw20302224

Calibrated On : July 3, 2023

Software Version : 9.0

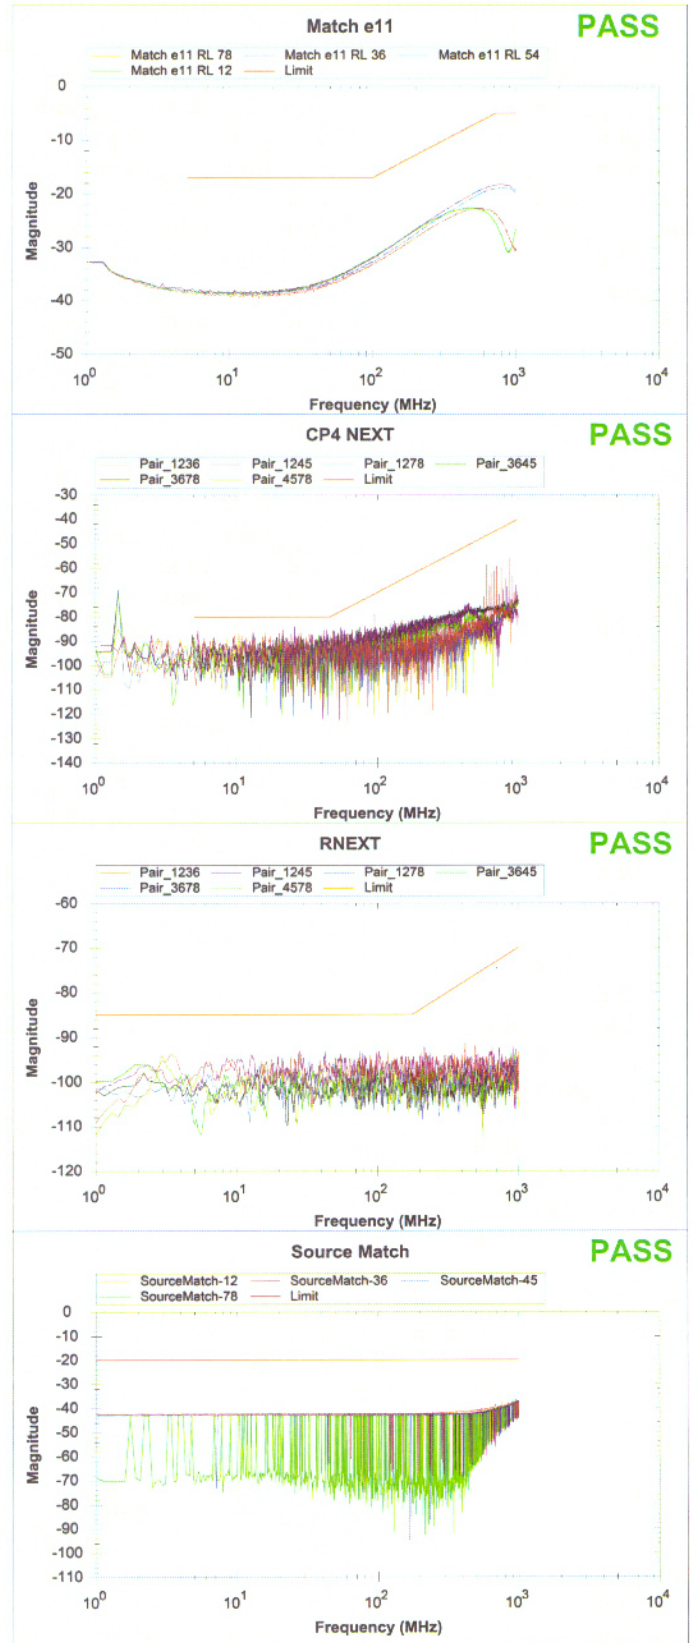
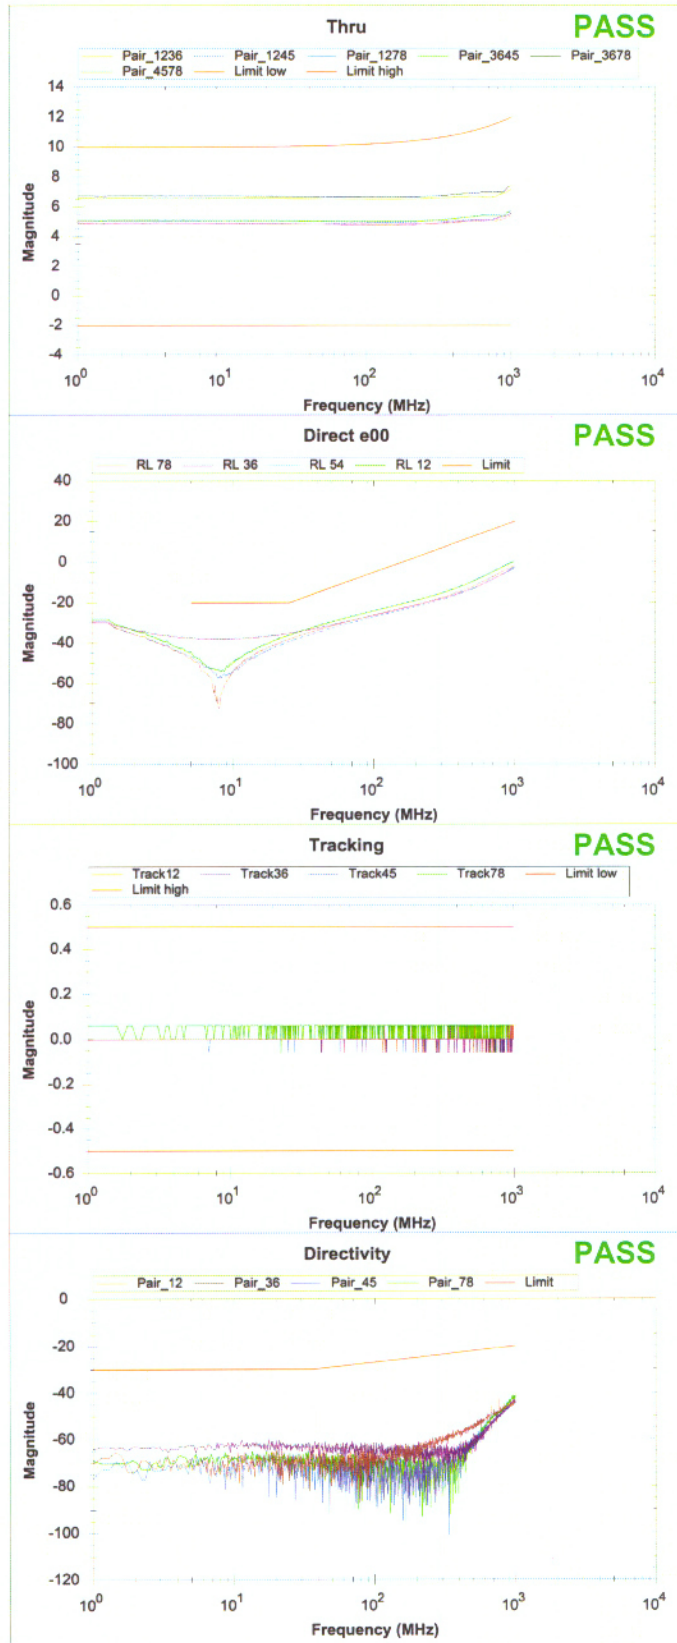




Serial No. jw20302223

Calibrated On : July 3, 2023

Software Version : 9.0

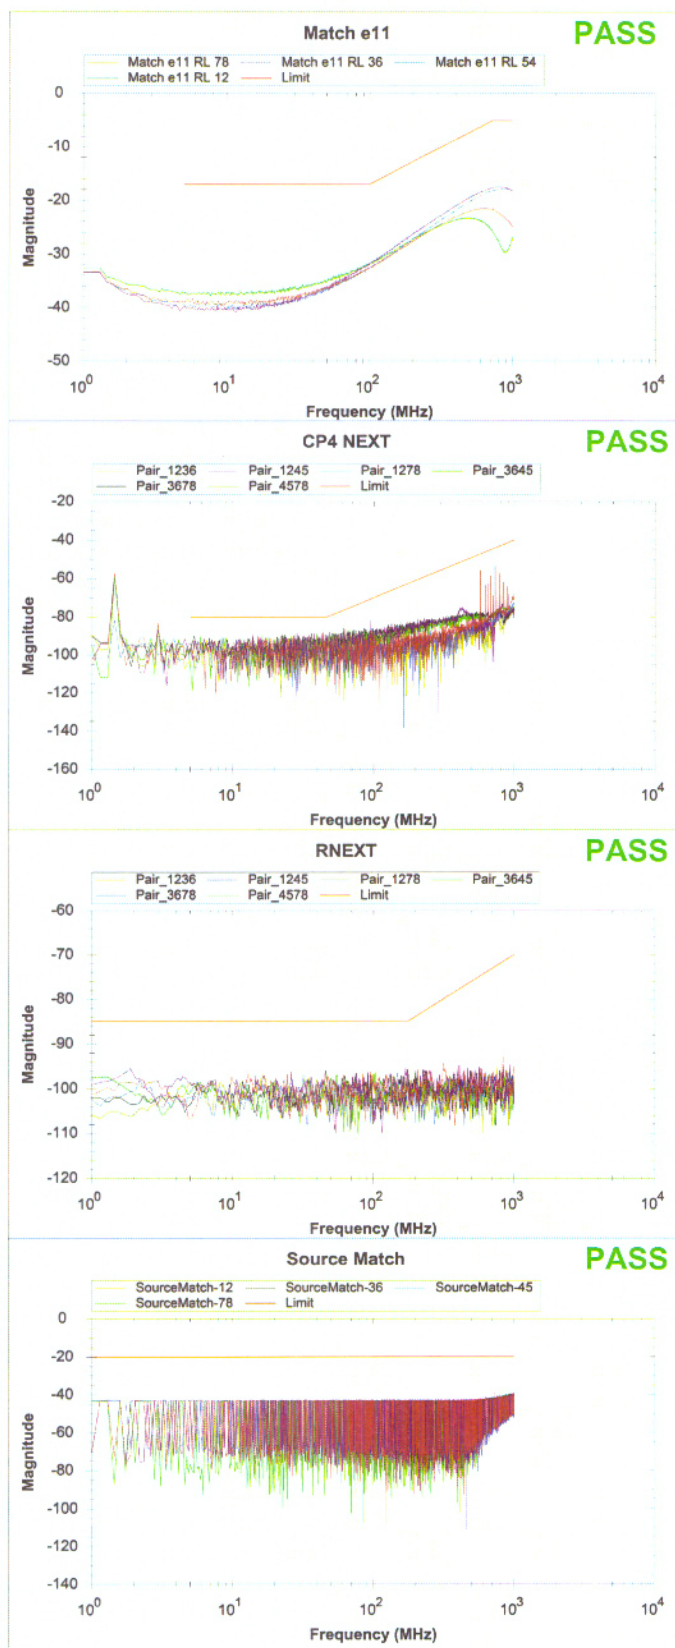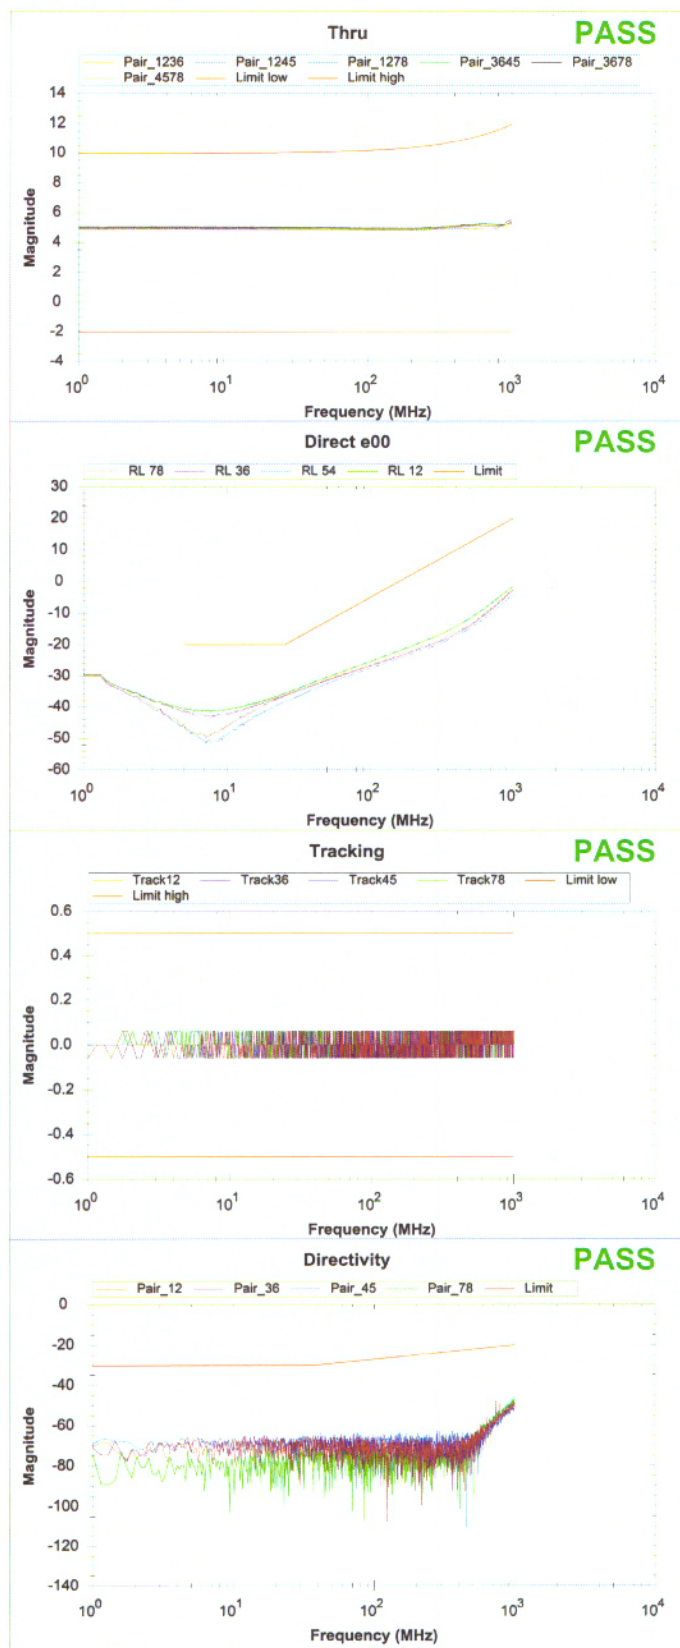



ELNEX
UL. WIERZBICKA 37
RADOM 26-600
PL

Equipment Service Report for SR Number: 10182323

CUSTOMER:	ELNEX	Order Number:	8596009309
MODEL:	21154432	PONumber:	VIAVI/06/2023-rev1
Inventory Item:	21154432	Job Type:	FIXED CAL
SerialNbr:	JW2030-2223	Warranty:	
Contract:		Calibration:	
Calibration Data:			

Customer's Request: TOP CAL-NGC-4500 LOCAL-JW2030-2223- CERTIFICATE - A-LAN Technologie

Physical Inspection: Good conditions

Received Accessories: BATTERY, T. BAG, ADAPTER, TOUCH PEN, SCREEN COVER

Troubleshooting: No trouble found

Repair Comments: Functional verification on ATE System performed conforms to all VIAVI specifications for this product

Calibration: Yes

Change Notice: NA

Upgrade: NA

Preventative Maintenance: General servicing and cleaning

Final Test: All test passed



ELNEX
UL. WIERZBIKA 37
RADOM 26-600
PL

Equipment Service Report for SR Number: 10182339

CUSTOMER:	ELNEX	Order Number:	8596009309
MODEL:	21168456	PONumber:	VIAVI/06/2023-rev1
Inventory Item:	21168456	Job Type:	FIXED CAL
SerialNbr:	JW2030-2224	Warranty:	
Contract:		Calibration:	
Calibration Data:			

Customer's Request: TOP CAL-NGC-4500 REMOTE-JW2030-2224- CERTIFICATE - A-LAN Technologie

Physical Inspection: Good conditions.

Received Accessories: BATTERY, ADAPTER, TOUCH PEN

Troubleshooting: Unit fails during calibration in CP4NEXT and RNEXT

Repair Comments: Measurement board exchanged. Calibration and functional verification on ATE
System performed conforms to all VIAVI specifications for this product

Calibration: Yes

Change Notice: NA

Upgrade: NA

Preventative Maintenance: General servicing and cleaning

Final Test: All test passed